

Class II composite resin restorations: faster, easier, predictable

R. D. Jackson¹

In brief

Explains how ongoing advances in instrumentation, materials and technology have solved the major challenges for placing Class II composite resin restorations.

Informs the reader of the current research in new bulk fill composites, validating their use and efficacy.

Provides clinical knowledge of a specific technique for placing a Class II composite restoration by viewing a case report.

Composite resin continues to displace amalgam as the preferred direct restorative material in developed countries. Even though composite materials have evolved to include nanoparticles with high physical properties and low shrinkage stress, dentists have been challenged to efficiently create quality, long lasting, predictable restorations. Unlike amalgam, composite resin cannot be condensed making the establishment of a predictable, proper contact more difficult. In addition, composite requires an understanding of adhesives and an appreciation for their exacting application. These facts combined with the precise adaptation and light-curing of multiple layers makes placement of quality Class II composite restorations tedious and time-consuming. For private practicing dentists, it can also have an effect on economic productivity. Clinicians have always wanted an easier, efficient placement technique for posterior composite restorations that rivals that for amalgam. It appears that advances in instrumentation, materials and technology have finally delivered it.

Introduction

Silver amalgam has been used in dentistry to restore posterior teeth for well over a century.¹ Preparing posterior teeth to receive amalgam fillings has universally been one of the first surgical procedures students perform in dental schools and the material has been the mainstay of services provided to patients well into the 1990s. The reasons for its popularity are many but primarily include: simplicity, predictability, longevity and low cost. Indeed, it is one of the most forgiving restorative materials in dentistry and its use is quickly and easily learned. Although isolation with a rubber dam is recommended and taught in dental schools, for the inexperienced, its placement can sometimes be the most difficult part of the

restorative procedure. For the newly qualified practitioner, rubber dam placement is likely the first step deleted from the restorative procedure as it is learned that skipping its use shortens the appointment time without seemingly affecting results.

Although amalgam has served dentistry well for a very long time, it is not a restorative material without drawbacks. Amalgam undergoes constant corrosion in the mouth, does not strengthen teeth, requires additional tooth structure removal for retention, and is not aesthetic. In addition, in spite of extensive evidence to the contrary, the potential effect of released mercury on patient health remains controversial.^{2–12} More recently, the environmental impact of waste mercury has added another dimension of concern over the use of amalgam in dentistry.¹³ This has led to limitations of use or even a ban of its use in some countries.^{14–16} In 2013 a global treaty was signed by 128 countries calling for the promotion of cost and clinically effective mercury-free fillings and, among other provisions, encourages professional organisations and dental schools to educate and train on the use of mercury-free alternatives.¹⁷ Currently, the obvious alternative material to use as a direct

restorative in posterior teeth is composite resin.¹⁸ This adhesively bonded material seals teeth, reinforces teeth, is more conservative since it does not require mechanical retention or specific preparation geometry, and satisfies patient desires for a natural looking restoration.^{19–26} Also, today's restorative composite resins are highly advanced materials with high micro and nano filler content which optimises high physical properties and increased wear resistance, a necessity for durable function over time.^{27–30} In fact, composite resin is already a significantly, if not dominantly, used restorative material for posterior teeth, particularly in developed countries.^{31–37} Its current popularity is confirmed by the fact that, in 2010, for dentists in the United States, placement of composite resin restorations exceeded amalgam fillings by a ratio of 2:1 and 1/3 of dentists reported not using amalgam at all.^{38,39} However, the transition for dentists from using amalgam to using composite resin hasn't been easy and dentists sometimes find posterior composite resin restorations, particularly of the Class II type, challenging to place. Therefore, the contradiction is that even though posterior composite resin restorations have become mainstream in many countries, dentists complain that placing

¹Fellow, American Academy of Cosmetic Dentistry, Madison, Wisconsin; Diplomate, American Board of Aesthetic Dentistry, Columbus, Ohio; Private Practice, Middleburg, Virginia, USA

Correspondence to: R. D. Jackson
Email: ron@ronjacksondds.com

Refereed Paper. Accepted 7 March 2016

DOI: 10.1038/sj.bdj.2016.856

©British Dental Journal 2016; 221: 623–631

them is exacting, tedious, time consuming and not always predictable.⁴⁰ The critique often cited is 'technique sensitive'.

The problems

The placement of a successful Class II composite resin restoration can be compared to the construction of a three legged stool. To function, all three legs have to be made correctly, that is, be exactly the same length, located in the right position and strongly attached to the stool. In the case of an economical and successfully placed Class II composite resin restoration, the three challenges (legs of the stool) are: 1) achievement of a predictable contact; 2) no or minor post-operative sensitivity of short duration; and 3) access to a simplified, faster and easier placement technique that delivers a consistent high quality result.

Contact

The contact problem stems from the fact that, unlike amalgam, composite resin cannot be condensed. To overcome this, dentists have resorted to using the wedge not only to seal the gingival margin in Class II preparations but to separate the teeth by pushing it hard into the embrasure space. This is arbitrary because the dentist can't tell if the teeth have truly separated enough to account for the thickness of the matrix band. Given the number of Class II restorations dentists place in a day, an occasional restoration with a light or no contact is an inevitable result. Lack of predictability alone heightens the stress for the clinician. The stress increases significantly in those instances where, at the end of the procedure, flossing reveals a light or no contact. The restoration will then have to be replaced or modified at considerable cost to the dentist and inconvenience to the patient.

Sensitivity

The first rule in dentistry is to not hurt the patient, or at the very least, to take steps to minimise discomfort. It is common for amalgam restorations to be sensitive to cold for several days following placement. However, post-operative sensitivity, particularly to chewing, for weeks or even months,⁴¹ has been an infrequent, but persistent, and unpredictable problem for clinicians following placement of posterior composite restorations.

Time and effort

Successful composite resin restorations require significantly more time and effort to place than amalgam restorations. The procedure includes: careful isolation, proper placement and light curing of the adhesive; placement and light curing of a low viscosity liner for intimate adaptation to the pulpal and gingival floors as well as into irregularities and undercuts; and then placement, adaptation and curing of multiple 2 mm layers of composite resin with the final layer requiring sculpting, finishing and polishing.⁴² The procedure begs for simplification. Finally, in circumstances where the fees are controlled by a third party, the profitability can be less for composite restorations as compared

to amalgam restorations because of the additional time required to perform them.²⁹

Solutions

Contact

It is clear that achieving a consistently good contact using composite resin requires a different approach than what has always worked well for amalgam. Fortunately, continued developments in matricing and contact forming instruments have eliminated the poor or open contact problem thereby making the achievement of a quality contact a predictable event. Examples of two well-designed sectional matrix systems with separating rings are shown in Figure 1. These systems are easy to use, have a short learning curve and yield excellent results. For this author, they are the default matrix for Class II restorations and work well for the vast majority of Class II cavities. They are only abandoned when clinical situations such as tipped teeth, teeth out of alignment, greater than normal intertooth distance, cuspal replacement, restoring distal surfaces of second molars etc, require a circumferential matrix. In these instances, there are a variety of different matrices in the marketplace that are used with a retainer. A few are shown in



Fig. 1 a) V3 and V4 sectional matrix systems by Triodent; b) Composi-tight sectional matrix system by Garrison Dental



Fig. 2 a) Convexi-T matrix by Clinician's Choice available thru Optident; b) Greater Curve matrix by Greater Curve; c) Pink Band matrix by Flycast Technologies



Fig. 3 a) Contact Pro2 by CEJ Dental; b) Trimax by ADdent; c) Preform by Garrison Dental

Figure 2. When a circumferential matrix is used, the wedge is inserted only to seal the gingival margin in the same manner as when placing amalgam. Instead of trying to separate the teeth with the wedge, contact forming instruments are used to achieve a contact. The instruments shown in Figure 3 are simple to use and yield consistently good contacts. Although what has been mentioned above is the author's approach to creating predictable quality contacts in Class II composite resin restorations, there are other systems of various designs available as well.

Sensitivity

A properly placed adhesive seals the dentine so most composite resin restorations will have no post-operative sensitivity at all. It is not unusual for some restored teeth to have a transient sensitivity to cold for a few days. This can result from brief pulpal hyperaemia because of presenting caries and/or trauma of the surgical procedure. However, what has plagued many dentists are patients reporting persistent pain on chewing. For this symptom, it is important to distinguish the type of post-operative sensitivity the patient is experiencing. If the restoration is high, the pain occurs every time the patient chews on the tooth. The patient quickly accommodates by chewing only on the opposite side. If irreversible pulpitis is not present, marking and adjusting the occlusion eliminates the pain. What has frustrated dentists is when patients state the pain is intermittent, occurs only when they 'hit a certain spot' and continues even when repeated adjustments result in light or no opposing contact. In this author's opinion, the cause of sensitivity in these instances is almost always lack of dentine seal.⁴³⁻⁴⁷ In the past, this type of problem has been ascribed to high shrinkage stress of the composite resin on cavity walls or the use of the phosphoric acid in the etch and rinse approach to adhesion. Shrinkage stress of the composite resin is an unlikely cause when proper incremental placement technique

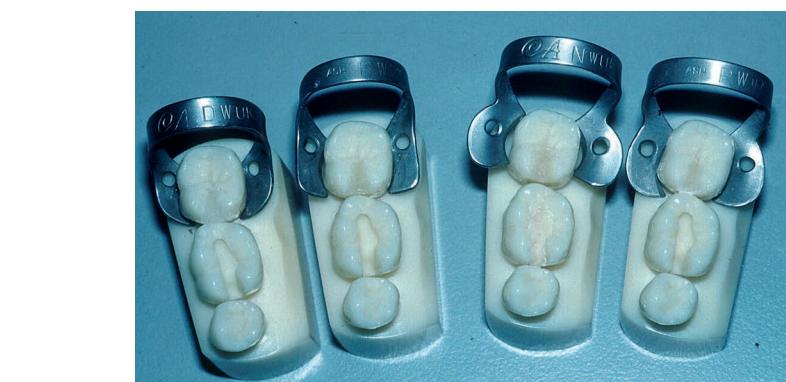


Fig. 4 Rubber dam clamps by Dentsply

is used and given that the higher filler content of contemporary composite resins has reduced volumetric shrinkage and resulting stress.⁴⁸ With regards to the use of phosphoric acid to condition dentine, controlled clinical trials have repeatedly shown little or no post-operative sensitivity whether the etch and rinse or a self-etch adhesive technique is used.^{43,49} Furthermore, anecdotal reports show the incidence of post-operative sensitivity declines as dentists master the more exacting technique required when using etch and rinse adhesives. For dentists who still have the occasional patient experiencing the intermittent post-operative sensitivity described above, switching to a self-etch adhesive along with selective etching the occlusal enamel with phosphoric acid, should solve the problem without compromising either the enamel or dentine bond.⁴⁴ Because contamination can be a cause of postoperative sensitivity as well as early failure of the restoration, it is important to note that isolation throughout the adhesive process and composite placement is mandatory. Although others may use a different approach, in this author's opinion, a well-placed rubber dam is still the optimal method for obtaining and maintaining the required isolation throughout the entire adhesive and composite placement procedure.

Working with a trained assistant, using a few simple, well designed clamps and practice makes the placement process very efficient (Fig. 4). The additional up front time involved in placement is more than made up by elimination of the cheek, tongue, gingiva and saliva from the operating field along with improved vision for the operating team.

Time and effort

Even with a consistent contact and elimination of post-operative sensitivity, dentists are still left with the considerable time and effort needed to insert, carefully adapt and then cure multiple layers of composite resin. In recent years manufacturers have introduced new 'bulk-fill' composite resins that allow dentists to place restorations in fewer increments. These materials fall into two categories: low viscosity (flowable) and high viscosity (sculptable). One unique system, SonicFill (Kerr) is a high viscosity composite resin, but, upon activation with a sonic handpiece, becomes a low viscosity material during the insertion phase. Manufacturers have altered the chemistry (for example, Tetric EvoCeram Bulk Fill [Ivoclar Vivadent -Schaan, Lichtenstein]), or polymer structure (for example, SDR Flow [Dentsply - York, Pennsylvania]), or

Table 1 "Bulk-Fill" Composite Resin Materials

	Materials	Composite type	Depth of cure*	Needs enamel replacement layer**	Low viscosity liner recommended
Low viscosity	SureFil SDR Flow [†] (Dentsply/Caulk)	Flowable	4 mm	Yes	No
	Tetric EvoFlow Bulk Fill [†] (Vivadent)	Flowable	4 mm	Yes	No
	Beautiful-Bulk Flowable [†] (Shofu)	Flowable	4 mm	Yes	No
	X-tra Base [†] (Voco)	Flowable	4 mm	Yes	No
	Venus Bulk Flow [†] (Heraeus Kulzer)	Flowable	4 mm	Yes	No
	Filtek Flow Bulk Fill [†] (3M/Espe)	Flowable	4 mm	Yes	No
	HyperFil [†] (Parkell)	Flowable	Infinite [‡]	Yes	No
	Fill Up [†] (Coltene)	Flowable	Infinite [‡]	Yes	No
High viscosity	BulkEZ [†] (Danville)	Flowable	Infinite [‡]	Yes	No
	Tetric EvoCeram Bulk Fill (Vivadent)	Sculptable	4 mm	No	Yes
	X-tra Fil (Voco)	Sculptable	4 mm	No	Yes
	Beautiful-Bulk Restorative (Shofu)	Sculptable	4 mm	No	Yes
	Filtek Bulk Fill Posterior Restorative (3M/Espe)	Sculptable	4 mm	No	Yes
	SonicFill [§] (Kerr)	Sculptable	5 mm	No	No

*Manufacturer's data. **Unless non-occlusal load bearing. †Dentine replacement (base). ‡Dual Cure. §Sonic delivery.

polymerisation kinetics (for example, SonicFill [Kerr - Orange, California]) of these advanced materials to control shrinkage stress and allow a high depth of cure up to 4 or 5 mm (Table 1).^{50–53}

Low viscosity materials act as a flowable base. They adapt very well to cavity walls and into undercuts and can be placed up to 4 mm in thickness. Dual cure flowables will cure at any depth. Since they are not sculptable and generally have low wear resistance to occlusal forces, these materials need to be covered or capped by one or two increments of a high viscosity material in all but very small cavities.⁵⁴ It should to be noted that some of these materials are very translucent, a fact that needs to be considered when covering preparations having dark internal stains. For clinicians, gaining adaptation with a single 4 mm base shortens placement time and effort.

The new high viscosity bulk-fill materials are shaded, sculptable, and, due to high filler content, have high strength and wear resistance. However, because adapting these materials intimately to pulpal floors, irregular preparations and undercuts can be challenging, lining the cavity with a low viscosity liner before placing the high viscosity material seems prudent.^{55–57} Once again, placing these materials in up to 4 mm increments saves time and effort for the clinician.

SonicFill (Kerr) seems to be in a class by itself. Due to its high filler content, this material is classified as a high viscosity material in the 'bulk-fill'

market. Its uniqueness lies in the fact that it is activated and injected into the cavity using a sonic handpiece. High frequency vibration of this material significantly lowers the viscosity, vibrates it into intimate contact with cavity walls and rapidly fills most cavities in seconds. No cavity liner is required for adaptation although the clinician can choose to apply one if desired. A depth of cure up to 5 mm means the majority of cavities can be filled in a single increment.^{52,58–61}

Although a specific handpiece is required, this system of composite resin placement seems to take the bulk fill concept one step further in speed and simplicity.

Case report

A patient presented with a leaking amalgam filling in a lower premolar that required replacement (Fig. 5). The patient was anaesthetised and a rubber dam with wax floss ligature was placed. After removing the amalgam, any base or liner and all caries, a sectional matrix (Triodont – Kati Kati, New Zealand) was placed. An appropriate sized wedge was inserted to seal the gingival margin. The stabilising/separating ring with V shaped tines was placed to adapt the matrix and create slight separation of the teeth (Fig. 6). Burnishing the matrix against the adjacent tooth established the size and location of the contact. The cavity measures 5 mm in depth and thus can be restored in a single increment of



Fig. 5 Premolar with failing amalgam and recurrent caries

SonicFill composite resin (Fig. 7). The adhesive was placed and cured according to the manufacturer's directions (Fig. 8). The handpiece has settings from 1 to 5 (slow to fast) to determine the extrusion rate desired for the composite resin material (Fig. 9). The extrusion rate should not be controlled through the rheostat. Complete activation of the rheostat is necessary for the material to achieve full liquefaction.⁵² A setting of 4 was chosen to fill this cavity. The tip is placed near the gingival floor of the proximal box (Fig. 10). It is withdrawn as the cavity is filled but kept in contact with the material at all times (Fig. 11). The cavity is filled in a few seconds (Fig. 12). A round end condenser or silicone tipped instrument is used to compress the material and simultaneously wipe away excess (Fig. 13). The material retains the activation energy for several minutes before returning back to a high viscosity state.



Fig. 6 Sectional matrix, wedge and stabilising/separating ring is placed. Contact is burnished

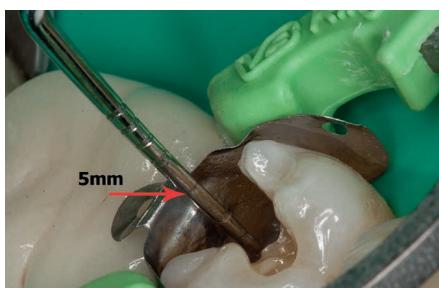


Fig. 7 Cavity depth from marginal ridge to gingival margin is slightly less than 5 mm



Fig. 8 The adhesive is placed and light cured



Fig. 9 SonicFill handpiece with composite resin filled tip attached. The numbers at the base of the handpiece regulate the extrusion speed of the material



Fig. 10 The tip is placed into the proximal box just above the gingival margin

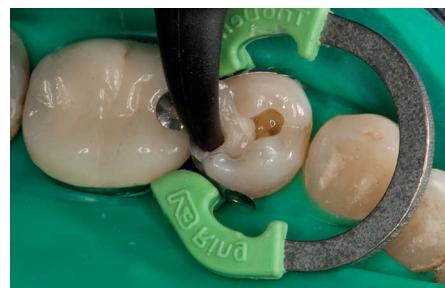


Fig. 11 The tip is withdrawn as the material fills the box. It is always kept in contact with the material



Fig. 12 The tip is moved in a straight line motion across the preparation filling the cavity. Waving the tip around could cause voids



Fig. 13 An instrument is used to compress the material and wipe away the excess



Fig. 14 Because the material retains the sonic energy for several minutes, it will feel soft but will not slump. Lack of stickiness allows quick and easy sculpting of anatomy



Fig. 15 A ten second cure from the occlusal surface is performed



Fig. 16 At this stage excess flash is removed easily



Fig. 17 Because curing is incomplete, occlusal flash can be feathered with a carbide bur. Using diamonds risks removing enamel, damaging margins and altering the occlusion

The liquefaction renders the material soft at this stage but it does not slump when sculpted and is non-sticky (Fig. 14). Using a light emitting diode curing light with an output above 1,000 mW/cm², the material is cured from the occlusal for

10 seconds (Fig. 15). Upon removal of the matrix assembly and wedge, a sharp number 12 blade on a scalpel handle is used to trim away any excess from the proximal margins (Fig. 16). It is the author's preferred technique to retain any bonded

occlusal flash and merely feather it with a 7,404 or 7,406 carbide finishing bur (Fig. 17). The cure is completed by applying ten additional seconds to



Fig. 18 a) The buccal surface is cured for 10 seconds; b) The lingual surface is cured for 10 seconds. The occlusal surface is cured an additional 10 seconds, giving a total cure of 40 seconds for the restoration. Curing times are based on using a high output ($>1,000 \text{ mW/cm}^2$) LED light

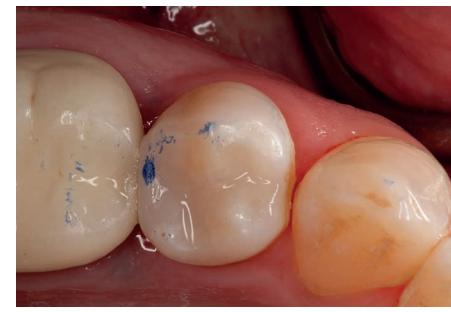


Fig. 19 After removing the ligature and rubber dam, the occlusion is marked and adjusted

both the buccal and lingual surfaces and again to the occlusal (Fig. 18). The rubber dam is removed, the occlusion is adjusted if necessary, and the restoration polished in the usual manner (Fig. 19). SonicFill has been shown to have high physical properties (flexural strength, hardness ratio, degree of conversion etc) compared to non-bulk-fill composite resin materials and its density and adaptation are evident on radiographs⁶² (Figs 20 and 21). A recently introduced newer version of the material (SonicFill 2) achieves higher polishability (Fig. 22).

Discussion

Composite resin is widely used for direct restoration of posterior teeth and because of advanced material development, increased understanding of proper adhesive technique as well as improved dentist training and experience in restoration placement, longevity of these restorations has increased significantly. Some clinical trials report the longevity of direct posterior composite restorations to be similar or even superior to that of amalgam restorations.^{63–67} Longevity can be further enhanced because composite resin restorations can often be easily repaired without replacing the entire restoration. This in turn reduces additional trauma to the tooth and cost to the patient.^{68,69} It appears that when using contemporary advanced composite formulas, longevity of restorations is mostly operator and patient dependent.⁶² Unlike clinical trials performed using strict protocols by calibrated operators, practice-based longitudinal studies still report amalgam fillings having somewhat better longevity than composite restorations.⁷⁰ It should be noted that in practice-based studies, restorations are sometimes performed by multiple clinicians with differing experience and training, using various techniques. In addition, the economic and time pressures inherent in private



Fig. 20 Five year post-operative image shows good margins and no evidence of wear. Because posterior restorations are always seen wet, the lack of high polish is not aesthetically critical for patients

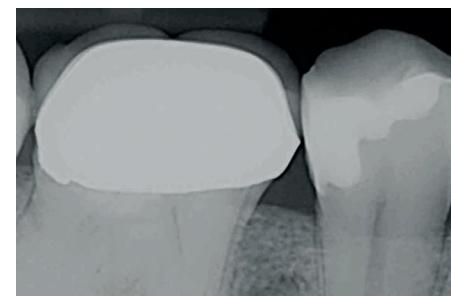


Fig. 21 The density and adaptation is evident on this 5-year post-operative radiograph. No liner was used



Fig. 22 Pre and post-operative views of the next generation composite resin material, SonicFill 2. Higher gloss is noted and even higher wear resistance is claimed due to the use of nano zirconia filler particles

practice compared to trials conducted in an academic setting can also affect outcomes. It is obvious that for private practicing dentists to economically achieve consistently good results, the entire process for placing posterior composite restorations has to be simpler, faster, and easier without compromising durability, adaptation, marginal integrity or any of the other parameters of a successful restoration. Innovations in matricing along with advancements and simplification of adhesives, have significantly improved predictable results for these two critical components of a successful Class II restoration. The introduction of newer

'bulk fill' composite resins appears to have completed the needed third leg of the triad. However, since these new materials break with the traditional protocol for layering composite resin in no more than 2 mm increments, the science needs to be examined to confirm that, in fact, they meet manufacturers' claims for low shrinkage stress and high depth of cure when placed in increments of 4 or, for some materials, 5 mm.

One of the reasons for layering traditional or universal composite resin in no more than 2 mm increments is to supposedly lower shrinkage stress and there is literature supporting this

technique.^{30,71} However, there is also research questioning the value of incremental placement in reducing shrinkage stress and at least one investigation concluded this technique actually increases it.^{72–77} Nevertheless, placing traditional restorative composites in 2 mm layers may still be required for purposes of good adaptation and to achieve adequate depth of cure. The current literature reporting on shrinkage stress for bulk-fill materials predominately shows these materials at 4 or 5 mm thicknesses to have similar or lower values when compared to 2 mm thicknesses of universal composites.^{78–81} In a comprehensive evaluation of bulk-fill versus traditional multi-increment composite resins carried out at the American Dental Association laboratory, shrinkage stress values for 9 out of 11 bulk fill materials tested were not significantly different than the two conventional composite resin controls. The value for X-trabase (Voco- Indian Land, South Carolina, USA) was significantly higher and SonicFill (Kerr) was significantly lower than all the other materials tested.⁴⁸ Another *in vitro* investigation examining gap formation at dentine margins of Class II restorations showed similar results for Tetric EvoCeram Bulk Fill (Ivoclar Vivadent - Schaan, Lichtenstein), SonicFill (Kerr) and SDR Flow (Dentsply) compared to a conventional layered composite (Tetric EvoCeram (Ivoclar Vivadent). The two low viscosity bulk-fills, x-trabase (Voco) and Venus Bulk Fill (Hereaus Kulzer – South Bend, Indiana, USA), showed larger gaps.⁸² Whether this difference would be clinically significant is not known. With minor difference for some products, *in vitro* studies on marginal adaptation/marginal integrity show similar results for bulk fill products (high and low viscosity) when compared to traditional layered controls.^{83–87} Overall, the data for the bulk fill materials seems to support manufacturers' claims that the modifications made in these materials have succeeded in controlling shrinkage stress to nearly the same or lesser amount than experienced with current conventional composites. Finally, in a recent investigation comparing an incrementally placed composite restoration (Point 4, Kerr) to a sonicated bulk fill (SonicFill, Kerr) restoration, the sonicated bulk fill composite resin showed significantly fewer voids.⁸⁸

There are two common methods used to measure depth of cure. An unsophisticated, but simple method that can be carried out by any dentist is the International Standards Organisation (ISO) #4049:2009.⁸⁹ This method cures a column of composite in a metal mould

from the top and scrapes away the soft, uncured composite from the bottom until reaching hard cured material. The depth of cure is then defined by dividing the remaining length of hard composite by two. Since this method does not actually measure polymerisation (carbon conversion) at any given depth, it is an approximation at best. Its underestimation of depth of cure was pointed out in an investigation by Tiba and colleagues into depth of cure for several bulk-fill materials and was presented at the International Association of Dental Research (IADR) meeting in 2013. The authors concluded their study with the following statement: 'This study shows some limitations of ISO 4049 for testing depth of cure in relation to the more important hardness ratio for bulk fill composite materials.'⁹⁰

Other investigations have also questioned the testing protocol and clinical relevancy of the ISO 4049 testing method.^{61,91} A second method used by many investigators for measuring depth of cure and referred to in the Tiba statement above, uses microhardness testing. It defines the depth of cure as the distance from the top of the cured column of composite to a point where the microhardness value is at least 80% of the top surface value.⁹² Hardness has been shown to correlate to polymerisation (80% bottom-to-top hardness equals 90% carbon conversion).⁹³ Since it indirectly measures actual polymerisation, the microhardness method for determining depth of cure seems more accurate and clinically relevant. When applying the 'scrape test' to various bulk fill materials, some have failed to meet manufacturers' claims except when tested using actual teeth instead of a metal mould.⁶¹ However, investigations using the more valid microhardness test have consistently shown bulk fill materials meeting or exceeding manufacturers' specifications.^{48,80,82,90,94–100} The manufacturer of SonicFill notes that measurements for shrinkage stress and depth of cure should be done on the activated material rather than the static material to accurately reflect the true values that would occur in clinical use.¹⁰¹

Since bulk fill composite resin materials are so new, long term clinical trials are lacking. Short term clinical trials, published and unpublished are just beginning to appear. Early data shows bulk fill materials performing clinically similar compared to 2 mm layered materials.^{102–104} Nevertheless, surveys show high early acceptance and strong growth in use among dentists in the marketplace.^{105,106} Given the number of posterior composite restorations dentists place in practice, this growth

would seem unlikely if these new materials and technologies weren't performing successfully.

Along with a more efficient placement technique, bulk fill materials may also reduce operator error. A university dental school study showed that new graduates achieved better margins and less gaps between layers using bulk fill techniques compared to conventional layered techniques.¹⁰⁷ This fact confirms that easier, simpler techniques lead to consistently better results.

Conclusion

The development of innovative sectional matrix systems and simplified universal adhesives, with or without selective etch, along with the advent of bulk fill composites, would seem to be a significant turning point in posterior direct restorative dentistry. This combination creates a streamlined, straight forward, faster, more efficient and economical placement technique with less effort than previous methods. Practicing dentists have always desired a less labour intensive clinical protocol for placing posterior composite resin restorations – one that was as easy and timely as amalgam. It appears it has finally arrived.

Competing interests

Dr Ron Jackson discloses that he acted as a consultant in the development of SonicFill™ and retains a financial interest.

- Black G V. Pathology of the hard tissue of the teeth. *Operative Dentistry*, Vol. 1 Chicago: Medico-Dental Publishing Company, 1908.
- Vimy M J, Boyd N D, Hopper D E, Lorscheider F L. Glomerular Filtration impairment by mercury released from dental 'silver' fillings in sheep. *Physiologist* 1990; **33**: 651.
- Enwonwu C O. Potential health hazard of use of mercury in dentistry: critical review of the literature. *Environ Res* 1987; **42**: 257–274.
- Mackert J R, Berglund A. Mercury exposure from dental amalgam fillings: absorbed dose and the potential for adverse health effects. *Crit Rev Oral Biol Med* 1997; **8**: 410–436.
- Bjorkman L, Paedersen N L, Lichtenstein P. Physical and mental health related to dental amalgam fillings in Swedish twins. *Community Dent Oral Epidemiol* 1996; **24**: 260–270.
- Mackert J R Jr., Leffell M S, Wagner D A, Powell B J. Lymphocyte levels in subjects with and without amalgam restorations. *JADA* 1991; **122**: 49–53.
- Koral S M. Mercury from Dental Amalgam: Exposure and Risk Assessment. *Compend Contin Educ Dent* 2013; **34**: 138–146.
- ADA Council on Scientific Affairs. Dental Amalgam: Update on Safety Concerns. *J Am Dent Assoc* 1998; **129**: 494–503.
- Ucar Y, Brantley W A. Biocompatibility of dental amalgams. *Int J Dent* 2011; 981595.
- Scientific Committee on Emerging and Newly Identified Health Risks, European Commission. Are dental fillings safe? Safety of dental amalgam and alternative dental restoration materials. European Commission. Available online at http://ec.europa.eu/health/scientific_committees/docs/citizens_dental_filling_en.pdf (accessed October 2016).

11. Homme K G, Kern J K, Haley B E et al. New Science challenges old notion that mercury dental amalgam is safe. *Biometals* 2014; **27**: 19–24.
12. Mutter J. Is dental amalgam safe for humans? The opinion of the scientific committee of the European Commission. *J Occup Med Toxicol* 2011; **6**: 2.
13. BIO Intelligence Service. Study on the potential for reducing mercury pollution from dental amalgam and batteries. Final report prepared for the European Commission – DG ENV. 2012. Available online at http://ec.europa.eu/environment/chemicals/mercury/pdf/final_report_110712.pdf (accessed October 2016).
14. Norwegian Ministry of the Environment and International Development, 2008.
15. Danish Ministry for Health, 2008.
16. Swedish Ministry of Health and Social Affairs, 2008.
17. Minamata Convention on Mercury. January 19 2013. Geneva, Switzerland.
18. Lynch C D, Opdam N J, Hickel R et al. Guidance on Posterior Resin Composites: Academy of Operative Dentistry – European Section. *J Dent* 2014; **42**: 377–383.
19. Coelho-De-Souza F H, Camacho G B, Demarco F F, Powers J M. Fracture resistance and gap formation of MOD restorations: influence of restorative technique, bevel preparation and water storage. *Oper Dent* 2008; **33**: 37–43.
20. Liberman R, Ben-Amar A, Gontar G, Hirsh A. The effect of posterior composite restorations on the resistance of cavity walls to vertically applied occlusal loads. *J Oral Rehab* 1990; **17**: 99–105.
21. McCulloch A J, Smith B G M. In Vitro Studies of cusp reinforcement with adhesive restorative material. *Brit Dent J* 1986; **161**: 450–452.
22. Fissore B, Nicholls J, Youdelis R. Load fatigue of teeth restored by a dentin bonding agent and a posterior composite resin. *J Prost Dent* 1991; **65**: 80–85.
23. Eakle W S. Fracture Resistance of teeth restored with Class II bonded composite resin. *J Dent Res* 1986; **65**: 149–152.
24. Macpherson L C, Smith B G N. Reinforcement of weakened cusps by adhesive restorative materials: an *in vitro* study. *Brit Dent J* 1995; **178**: 341–344.
25. Lynch C D, Frazier K B, McConnel R J et al. Minimally invasive management of dental caries. *J Am Dent Assoc* 2011; **142**: 612–620.
26. de Freitas C R, Miranda M I, de Andrade M R et al. Resistance to maxillary premolar fractures after restoration of class II preparations with resin composite or ceromer. *Quint Int* 2002; **33**: 589–594.
27. Klapdohr S, Moszner N. New inorganic components for dental filling composites. *Monatshefte für Chemie* 2005; **136**: 21–45.
28. Leprince J G, Palin W M, Hadis M A, Devaux J, Leloup G. Progress in dimethacrylate-based dental composite technology and curing efficiency. *Dent Mater* 2013; **29**: 139–156.
29. Christensen G J. Class II Resins: Nanofill Brands as Group Show Best Performance Yet. *Clinician's Report* 2014; **7**.
30. Ferracane J L. Resin composite-state of the art. *Dent Mater* 2011; **27**: 29–38.
31. Sunnegardh-Gronberg K, van Dijken J W V, Funegardh U, Lindberg A, Nilsson M. Selection of dental materials and longevity of replaced restorations in Public Dental Health clinics in northern Sweden. *J Dent* 2009; **37**: 673–678.
32. Mitchell R J, Koike M, Okabe T. Posterior amalgam restorations – usage, regulation and longevity. *Dent Clin North Am* 2007; **51**: 573–589.
33. Opdam N J M, van de Sande F H, Bronkhorst E et al. Longevity of Posterior composite restorations: a systematic review and meta-analysis. *J Dent Res* 2014; **93**: 943–949.
34. Burke F J. Amalgam to tooth-coloured materials: implications for clinical practice and dental education. Governmental restrictions and amalgam usage survey results. *J Dent* 2004; **32**: 343–350.
35. Lund A. In your dental practice, is dental amalgam still the restorative material of choice? *J Am Dent Assoc* 2002; **133**: 1046.
36. Burke F J, McHugh S, Hall A C, Randall R, Widstrom E, Forss H. Amalgam and composite use in UK general dental practice in 2001. *Br Dent J* 2003; **194**: 613–618.
37. Christensen G J, Child P L Jr. Has resin-based composite replaced amalgam? *Dent Today* 2010; **29**: 108, 110.
38. Clinical Research Associates CRA Newsletter. Clinician's Preferences 2001 #15, CRA Newsletter. 2001: 3.
39. Christensen G J. Should resin-based composite dominate restorative dentistry today? *J Am Dent Assoc* 2010; **141**: 1490–1493.
40. Gilmour A S, Latif M, Addy L D, Lynch C D. Placement of posterior composite restorations in United Kingdom dental practices: techniques, problems, and attitudes. *In Dent J* 2009; **59**: 148–154.
41. Briso A L F, Mestreiner G, Delico R H, et al. Clinical assessment of post-operative sensitivity in posterior composite restorations. *Oper Dent* 2007; **32**: 421–426.
42. Burke F T J, Shortall A C C. Successful Restoration of load-bearing cavities in posterior teeth with direct-replacement resin-based composite. *Dent Update* 2001; 388–398.
43. Swift E. Ask the Experts: Dentin/Enamel Bonding. *J Esth Rest Dent* 2010; **22**: 352–353.
44. Van Meerbeek B, Yoshihara K, Yoshida Y, Mine A, De Munck J, Van Landuyt K L. State of the art self-etching adhesives. *Dent Mater* 2011; **27**: 17–28.
45. Loguercio A et al. Effect of Solvent removal on adhesive properties of simplified etch-and-rinse systems and on bond strengths to dry and wet dentin. *J Adhes Dent* 2009; **11**: 213–219.
46. Peumans M, Kanumilli P, DeMunck J et al. Clinical effectiveness of contemporary adhesives: a systematic review of current clinical trials. *Dent Mater* 2005; **21**: 864–881.
47. Van Meerbeek B, DeMunck J, Yoshida Y et al. Adhesion to Enamel and Dentin: Current status and future challenges. *Oper Dent* 2003; **28**: 215–235.
48. Tiba A, Zeller G G, Estrich C G, Hong A. A laboratory evaluation of bulk-fill versus traditional multi-increment-fill resin-based composites. *J Am Dent Assoc* 2013; **8**: 13–17.
49. Perdigão J, Geraldini S, Hodges J S. Total-etch versus self-etch adhesive effect on post-operative sensitivity. *J Am Dent Assoc* 2003; **134**: 1621–1629.
50. Tetric EvoCeram Bulk Fill- Scientific Documentation. Ivoclar Vivadent.
51. SDR Flow – Scientific Documentation., Dentsply.
52. Sonicfill – Scientific Documentation. Kerr.
53. Al-Ahdal K, Ilie N, Silikas N, Watts D C. Polymerization kinetics and impact of post polymerization on the degree of conversion of bulk-fill resin-composite at clinically relevant depth. *Dent Mater* 2015; **31**: 1207–1213.
54. Ilie N, Bucuta S, Draenert M. Bulk-fill resin-based composites: an *in vitro* assessment of their mechanical performance. *Oper Dent* 2013; **38**: 618–625.
55. Agarwal R S, Hiremath H, Agarwal J, Garg A. Evaluation of cervical margin and internal adaptation using newer bulk fill composites: An *in vitro* study. *J Conserv Dent* 2015; **18**: 56–61.
56. Opdam N J M, Roeters J J M, Peters T C R B, Burgersdijk R C W, Teunis M. Cavity wall adaptation and voids in adhesive Class I resin composite restorations. *Dent Mater* 1996; **12**: 230–235.
57. Chuang S F, Jin Y T, Liu J K, Chang Ch, Shieh D B. Influence of flowable composite lining thickness on Class II composite restorations. *Oper Dent* 2004; **29**: 301–308.
58. Yapp R, Baumann A, Powers J M. Comparative curing and thermal properties of demi ultra LED curing light. Research report – number 58. *Dent Advisor* 2014. Available online at www.dentaladvisor.com/publications/research-reports/comparative-curing-and-thermal-properties-of-demi-ultra-led-curing-light.pdf (accessed July 2014).
59. Christensen G. Advantages and challenges of bulk-fill resins. *Clin Rep* 2012; **5**: 1–2.
60. Hansen E K, Asmussen E. Visible-light curing units: correlation between depth of cure and distance between exit window and resin surface. *Acta Odontol Scand* 1997; **55**: 162–166.
61. Tiba A, Vinh R, Estrich C. Clinically relevant measurements of depth of cure of bulk-fill composites. IADR March 2015, Boston, Massachusetts.
62. Leprince J G, Palin W M, Vanacker J, Sabbagh J, Devaux J, Leloup G. Physico-mechanical characteristics of commercially available bulk-fill composites. *J Dent* 2014; **42**: 993–1000.
63. Demarco F F, Correa M B, Cenci M S, Moraes R R, Opdam N J. Longevity of posterior composite restorations: not only a matter of materials. *Dent Mater* 2012; **28**: 87–101.
64. Heintze S D, Rousson V. Clinical effectiveness of direct Class II restorations – a meta-analysis. *J Adhes Dent* 2012; **14**: 407–431.
65. Opdam N J, van de Dande F H, Bronkhorst E et al. Longevity of posterior composite restorations: a systematic review and meta-analysis. *J Dent Res* 2014; **93**: 943–949.
66. Opdam N J M, Bronkhorst E M, Loomans B A C, Huysmans M C. 12-year survival of composite vs. amalgam restorations. *J Dent Res* 2010; **89**: 1063–1067.
67. Cetin A R, Unlu N, Cobanoglu N. A five-year clinical evaluation of direct nanofilled and indirect composite resin restorations in posterior teeth. *Oper Dent* 2013; **38**: E31–E41.
68. Fernandez E, Martin J, Vildosola P, Oiveira Junior O B et al. Can repair increase the longevity of composite resins? Results of a 10 year clinical trial. *J Dent* 2015; **43**: 279–286.
69. Opdam N J M, Bronkhorst E M, Loomans B A C, Huysmans M C. Longevity of repaired restorations: A practice based study. *J Dent* 2012; **40**: 829–835.
70. Kopperud S E, Bjorg Tveit A, Gaarden T, Sandvik L, Espelid I. Longevity of posterior dental restorations and reasons for failure. *Eur J Oral Sci* 2012; **120**: 539–548.
71. Park J, Chang J, Ferracane J L, Lee I B. How should composite be layered to reduce shrinkage stress incremental or bulk filling. *Dent Mater* 2008; **24**: 1501–1505.
72. Versluis A, Douglas W H, Cross M, Sakaguchi R L. Does an incremental filling technique reduce polymerization shrinkage stress. *J Dent Res* 1996; **75**: 871–878.
73. El-Badrawy W, Jafarbour S, Jazi H S, McComb D. Effect of Composite Insertion technique on cuspal deflection using *in vitro* simulation model. *Oper Dent* 2012; **37**: 399–395.
74. Rees J S, Jagger D C, Williams D R, Brown G, Duguid W. A reappraisal of the incremental packing technique for light cured composite resins. *J Oral Rehab* 2011; **31**: 81–84.
75. Campodonico C E, Tantbirojn D, Olin Ps, Versluis A. Cuspal deflection and depth of cure in resin-based composite restorations filled by using bulk, incremental and transstooh-illumination techniques. *J Am Dent Assoc* 2011; **142**: 1176–1182.
76. Idriss S, Habib C, Abduljabbar T et al. Marginal adaptation of class II resin composite restorations using incremental and bulk placement techniques: an ESEM study. *J Oral Rehabil* 2003; **30**: 1000–1007.
77. Braga R R, Ballester Ry, Ferracane J L. Factors involved in the development of polymerization shrinkage stress in resin-composites: a systematic review. *Dent Mater* 2005; **21**: 962–970.
78. El-Damanhoury H M, Platt J A. Polymerization Shrinkage Stress kinetics and related properties of bulk-fill resin composites. *Oper Dent* 2014; **39**: 374–382.
79. Kim R J Y, Kim Y J, Choi N S, Lee I B. Polymerization shrinkage, modulus, and shrinkage stress related to tooth-restoration interfacial debonding in bulk-fill composites. *J Dent* 2015; **43**: 430–439.
80. Olafsson V G. Effect of Composite Type and Placement Technique on Shrinkage Stress; IADR Boston Massachusetts, March 2015. #2198.
81. Rosato C M P, Bicalho A A, Verissimo C et al. Mechanical properties, shrinkage stress, cuspal strain and fracture resistance of molars restored with bulk-fill composites and incremental filling technique. *J Dent* 2015; **43**: 1520–1528.
82. Benetti A R, Havndrup-Paedersen C, Honoure D, Paedersen M K, Pallesen U. Bulk-Fill resin composites: polymerization contraction, depth of cure and gap formation. *Oper Dent* 2015; **40**: 190–200.
83. Campos E A, Ardu S, Lefever D, Jasse F F, Bortolotto T, Krejci I. Marginal adaptation of class II cavities restored with bulk-fill composites. *J Dent* 2014; **42**: 575–581.
84. Agarwal R S, Hiremath H, Agarwal J, Garg A. Evaluation of cervical marginal and internal adaptation using newer bulk fill composites: an *in vitro* study. *J Conserv Dent* 2015; **18**: 56–61.
85. Orlowski M, Tarczydlo B, Chalas R. Evaluation of marginal integrity of four bulk-fill dental composite materials: *in vitro* study. *Sci World Journal* 2015; **2015**: DOI: 10.1155/2015/701262
86. Furness A, Tadros M Y, Looney S W, Rueggeberg F A. Effect of bulk/incremental fill on internal gap formation of bulk-fill composites. *J Dent* 2014; **42**: 439–449.

87. Haak R, Naeke T, Pfeffer M, et.al. Adaptation of High-Viscosity Bulk-fill Composites in Class II Cavities; IADR Boston Massachusetts, March 2015. #651.
88. Jarisch, J, Lien W, Guevara P H, Greenwood W J, Dunn W J. Microcomputed tomographic comparison of posterior composite resin restorative techniques: sonicated bulk fill versus incremental fill. *Gen Dent* 2016; 20–24.
89. International Standard ISO 4049: 2009. Dentistry-Polymer-based restorative materials. Geneva: ISO.
90. Tiba A, Hong A, Zeller G. Examining the Depth of Cure for Bulk Fill Composite Materials, IADR Seattle Washington, March 2013. #2435.
91. Vogel K. Factors that Influence Depth of Cure Measurement According to ISO 4049, IADR September 2014 #502.
92. Watts D C, Amer O, Combe E C. Characteristics of visible-light activated composites. *Brit Dent J* 1984; **156**: 209–215.
93. Bouschlicher M R, Rueggeberg F A, Wilson B M. Correlation of bottom-to-top surface microhardness and conversion ratios of various resin composite compositions. *Oper Dent* 2004; **29**: 698–704.
94. Ilie N, Kefler A, Durner J. Influence of various irradiation processes on the mechanical properties and polymerization kinetics of bulk fill resin based composites. *J Dent* 2013; **41**: 695–702.
95. Alshali R Z, Silikas N, Satterthwaite J D. Degree of conversion of bulk fill compared to conventional resin-composites at two time intervals. *Dent Mater* 2013; **29**: e213–e217.
96. Czasch P, Ilie N. In vitro comparison of mechanical properties and degree of cure of bulk fill composites. *Clin Oral Investig* 2013; **17**: 227–235.
97. Bucuta S, Ilie N. Light transmittance and micro-mechanical properties of bulk fill vs. conventional resin based composites. *Clin Oral Investig* 2014; **18**: 1991–2000.
98. Zorzin J, Maier E, Harre S et al. Bulk-fill resin composites: Polymerization properties and extended light curing. *Dent Mater* 2015; **31**: 293–301.
99. Alshali R Z, Salim N A, Satterthwaite J D, Silikas N. Post-irradiation hardness development, chemical softening, and thermal stability of bulk-fill and conventional resin-composites. *J Dent* 2015; **43**: 209–218.
100. Alrahlah A, Silikas, Watts D C. Post-cure depth of cure of bulk fill dental resin-composites. *Dent Mater* 2014; **30**: 149–154.
101. Personal Communication. Dreschler U, Senior Research Scientist, Kavo Kerr. Orange, California.
102. van Dijken J W V, Pallesen U. Randomized 3-year clinical evaluation of class I and II posterior resin restorations placed with a bulk fill resin composite and a one-step self-etching adhesive. *J Adhes Dent* 2015; **17**: 81–88.
103. Ernst C P. Random Split Mouth Trial. Dept Oper Dent Johannes Gutenberg University Mainz, Germany, (unpublished).
104. Geissberger M, Kachalia P. University of Pacific School of Dentistry June 2011, Clinical Evaluation of Restorations using a New Composite Material and Oscillating Handpiece and Comparing it with Traditional Composite Material and Placement Technique (unpublished).
105. Restorative Survey, Dentaltown March, 2015 pp. 58. Available online at www.dentaltown.com/dentaltown/article.aspx?i=385&aid=5269 (accessed November 2016).
106. Restorative Dental Survey. Posterior Composites, Dental Products Report. April 2015; 32–33. http://www.dentalproductsreport.com/files/files/dpr0415_ezine.pdf (accessed November 2016).
107. McConnell R, Lappin M. Comparison of Composite Placement Techniques by Recently Qualified Dental Practitioners, IADR March 2015 Boston, Massachusetts.